




## User Manual

# ClickTech Sensitive EdU Cell Proliferation Kit for High-throughput Screening

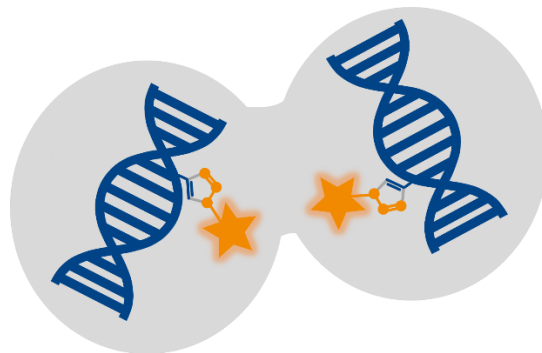

Ordering information  
(for detailed kit content see **Table 2**)

**EdU DetectPro HTS Kits ready for 2 x 96 well plate assays:**

Product number	EdU	Used fluorescent dye
BCK-EdUPro488HTS2	2 mL	Eterneon <sup>2</sup> GREEN Azide (Enhancer system – incl. FITC alternative)
BCK-EdUPro555HTS2	2 mL	Eterneon <sup>2</sup> YELLOW Azide (Enhancer system – incl. Cy3 alternative)

**EdU DetectPro HTS Kits ready for 4 x 96 well plate assays:**

Product number	EdU	Used fluorescent dye
BCK-EdUPro488HTS4	2 x 2 mL	Eterneon <sup>2</sup> GREEN Azide (Enhancer system – incl. FITC alternative)
BCK-EdUPro555HTS4	2 x 2 mL	Eterneon <sup>2</sup> YELLOW Azide (Enhancer system – incl. Cy3 alternative)

For References, FAQs and ordering please see online or contact us:

online: [www.baseclick.eu](http://www.baseclick.eu)  
orders: [orders@baseclick.eu](mailto:orders@baseclick.eu)  
support: [support@baseclick.eu](mailto:support@baseclick.eu)  
phone: +49 89 9699 3401  
fax: +49 89 9699 4696

## ClickTech Sensitive EdU HTS Kit

### Introduction and product description:

The detection of cell proliferation is of utmost importance for assessing cell health, determining genotoxicity or evaluating anticancer drugs. This is normally performed by adding nucleoside analogues like [<sup>3</sup>H]thymidine or 5-bromo-2'-deoxyuridine (BrdU) to cells during replication, and their incorporation into DNA is detected or visualized by autoradiography or with an anti-BrdU-antibody respectively. Both methods exhibit several limitations. Working with [<sup>3</sup>H]thymidine is troublesome because of its radioactivity. Autoradiography is slow and thus not suitable for rapid high-throughput studies. The major disadvantage of BrdU staining is that the double-stranded DNA blocks the access of the anti-BrdU antibody to BrdU units. Therefore, samples have to be subjected to harsh denaturing conditions resulting in degradation of the structure of the specimen.

### For research use only.


Information in this document is subject to change without notice. baseclick GmbH assumes no responsibility for any errors that may appear in this document.

baseclick GmbH disclaims all warranties with respect to this document, expressed or implied, including but not limited to those of merchantability or fitness for a particular purpose. In no event shall baseclick GmbH be liable, whether in contract, tort, warranty, or under any statute or on any other basis for special, incidental, indirect, punitive, multiple or consequential damages in connection with or arising from this document, including but not limited to the use thereof.

Please read the material safety data sheets (MSDS) provided for each product/component.

**Literature Citation:** When describing a procedure for publication using this product, please refer to it as *baseclick ClickTech Sensitive EdU HTS Kit*.

How the **enhanced Sensitive EdU cell proliferation** assay works

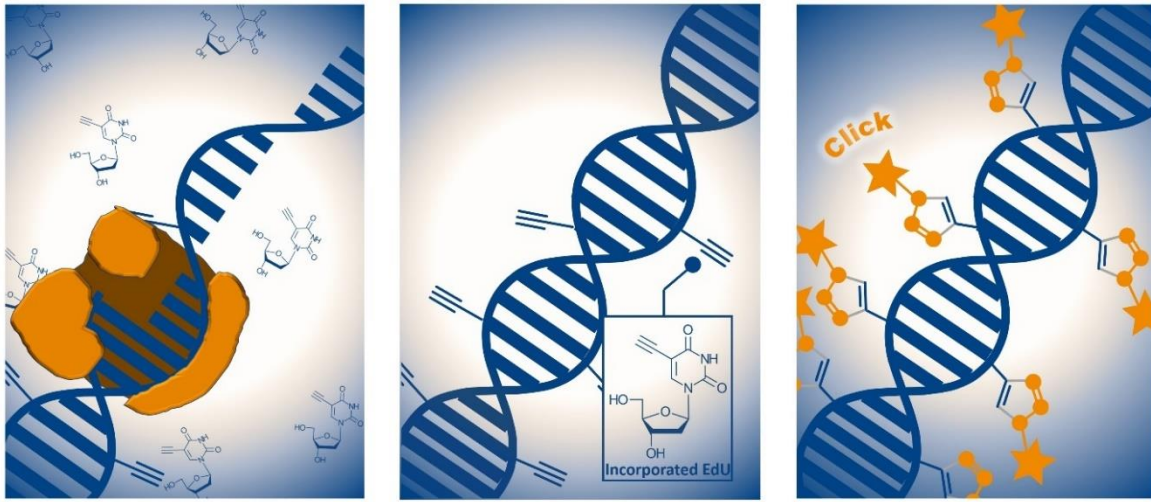

The baseclick **Sensitive EdU** overcome these limitations, providing a superior alternative to BrdU and [<sup>3</sup>H]thymidine assays for measuring cell proliferation.

Just as in the traditional EdU proliferation kits from baseclick, also here EdU (5-ethynyl-2'-deoxyuridine) (a nucleoside analog to thymidine) is incorporated into DNA during active DNA synthesis. In contrast to BrdU assays, the **Sensitive EdU** are not antibody based and therefore do not require DNA denaturation for detection of the incorporated nucleoside. Instead, the **Sensitive EdU** utilize click chemistry for detection in a variety of dye fluorescent readouts. Furthermore, the streamlined detection protocol reduces both the total number of steps and significantly decreases the total amount of time.

The simple click chemistry detection procedure is complete within 30 minutes and is compatible with multiplexing for content and context-rich results.

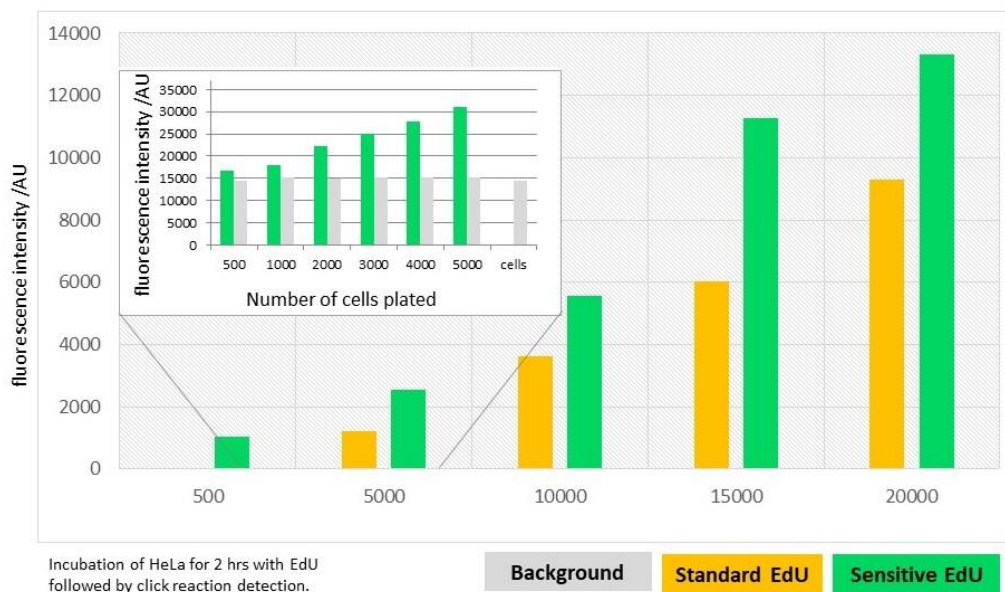


Figure 1: Comparison of the fluorescence intensities between the standard EdU Kit and the Sensitive EdU Kit.

The baseclick *Sensitive EdU HTS Kit* can be used with antibodies against surface and intracellular markers. To ensure the compatibility of your reagent or antibody, please refer to **Table 1**.

Table 1: EdU detection dye compatibility

Fluorescent molecule	Compatibility*
Organic dyes such as Fluorescein and Alexa dyes	Compatible
PerCP, Allophycocyanin (APC) and APC-based tandems	Compatible
R-phycoerythrin (R-PE) and R-PE based tandems	Use R-PE and R-PE based tandems <b>after</b> the EdU detection reaction
Quantum Dots	Use Quantum Dots <b>after</b> the EdU detection reaction
Fluorescent proteins (e.g. GFP)	Use anti-GFP antibodies** <b>before</b> the EdU detection reaction or use organic dye-based reagents for protein expression detection

\* Compatibility indicates which involved components are unstable in the presence of copper catalyst for the EdU detection reaction (either the fluorescent dye itself or the detection method).

\*\* The resulting fluorescence intensity depends strongly on the antibody manufacturer and target. Internal tests have shown a generally good fluorescence amount for rabbit and chicken anti-GFP and a very low fluorescence amount for mouse monoclonal antibodies. This can be understood as a general guideline but results may still greatly vary depending on the individual chosen antibody.

#### Cautions:

*The rinse buffer (Component R)*: contains hazardous components. Use with appropriate precautions. Keep away from acids to avoid dangerous gases.



Handle reagents containing the rinse buffer using equipment and practices appropriate for the hazards posed by such materials. Use gloves. Dispose of the reagents in compliance with all related local arrangements.

This solution is stored at RT and will crystallize at lower temperatures. If crystallized, the solution has to be brought to RT, mixed thoroughly and can then, once homogeneously dissolved, be used without further considerations. The activity of this compound is not affected hereby.

**MSDS:** the appropriate MSDS can be downloaded from our website [www.baseclick.eu](http://www.baseclick.eu).

## 1. Materials provided with the Kit and storage conditions

Table 2: Contents of the kit and storage conditions

Color code	Amount for 2 assays/well plates	Amount for 4 assays/well plates	Component	Component long term storage	Kit short term storage*
<b>Component E</b> yellow	2 mL	2 x 2 mL	5-Ethynyl-deoxyuridine (5-EdU)	- 20 °C	2 - 8 °C Dark Do not freeze Dry
<b>Component D</b> red	1 x 60 µL	2 x 60 µL	<ul style="list-style-type: none"> <li>Eterneon<sup>2</sup> GREEN Azide (BCK-EdUPro-HTS488)</li> <li>Eterneon<sup>2</sup> YELLOW Azide (BCK-EdUPro-HTS555)</li> </ul>	- 20 °C dark	
<b>Component RP</b>	40 mL	40 mL	Reaction Buffer	2 - 8 °C	
<b>Component C</b> green	1 mL	2 mL	Reactor System	2 - 8 °C	
<b>Component B</b>	200 mg	2 x 200 mg	Buffer additive	2 - 8 °C/ - 20 °C**	
<b>Component R</b>	6 mL	2 x 6 mL	Rinse buffer (10x)	RT	

\* This kit is stable up to 1 year after receipt, when stored as directed.

\*\* When dissolved the component has to be kept at - 20 °C for long-term storage. Prepare aliquots to avoid too many freeze and thaw cycles; if the solution starts to develop a brown colour, it has degraded and should be discarded.

## 2. Required Material and Equipment not included in this kit


- Adherent cells
- Reaction tubes (size depends on the volume of reaction cocktail needed)
- Buffered saline solution, such as PBS, D-PBS or TBS
- Fixative solution (4% Paraformaldehyde in PBS)
- Permeabilization solution optimised for your cell line (for example, 0.5% Triton® X-100 in PBS, or a 0.5% saponin-based solution)
- Appropriate cell culture medium
- 1% BSA (bovine serum albumin) in PBS, pH 7.1 - 7.4
- Deionized water or 18 MΩ purified water

### 3. Workflow

The following protocol was developed using a final EdU concentration of 10  $\mu$ M and can be adapted for any cell type. There are many factors, which can influence the labeling such as the growth medium, the density and the type of cells. To determine the optimal concentration for your experiment, a range of EdU concentrations should be tested for your cell type and experimental conditions.

Principally, a similar concentration to BrdU can be used for EdU as a starting point. Heparin can be used as anticoagulant for collection, if a whole blood sample is used.

#### Workflow scheme for the *Sensitive EdU HTS Assay*

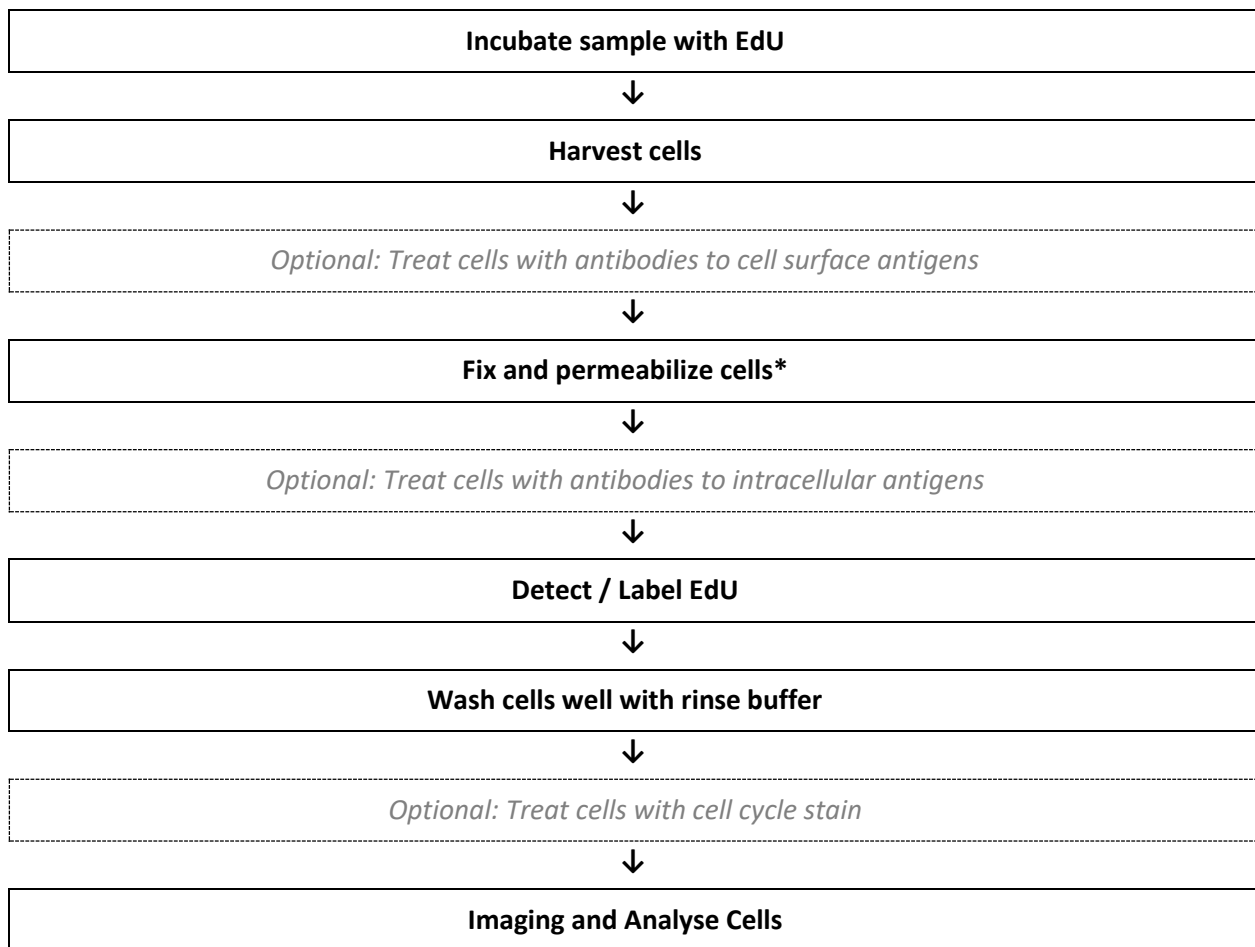

\* At this point the sample can be stored safely

## 4. Preparation of the stock solutions

- 4.1. Allow all vials to warm to room temperature before opening.
- 4.2. For the preparation of a 20  $\mu$ M stock solution of EdU (2x EdU), add the appropriate amount of aqueous solution (1x PBS) to EdU (**component E**) according to **Table 3** and mix until the compound is completely dissolved. After use, store any remaining solution at  $-20\text{ }^{\circ}\text{C}$ . When stored as directed, this stock solution is stable for up to one year.

Table 3: Amounts of aqueous solution needed to dissolve EdU to a final concentration of 20  $\mu$ M

EdU DetectPro HTS Kit	20X EdU solution	Dilution volume of 1x PBS
2 x 96 well plates	2 mL	18 mL
4 x 96 well plates	4 mL	36 mL

- 4.3. For the preparation of a stock solution of the buffer additive, add the appropriate amount of deionized water (see **Table 4**) to the **component B** and mix until the compound is dissolved completely. After use, store any remaining solution at  $-20\text{ }^{\circ}\text{C}$ . When stored as directed, this stock solution is stable for up to 6 months. We recommend preparing aliquots to avoid repeated freeze and thaw cycles!

Table 4: Amounts of aqueous solution needed to dissolve the buffer additive to the final work solution

EdU DetectPro HTS Kit	Buffer additive (solid)	Dilution volume of deionized water
2 x 96 well plates	200 mg	2.5 mL
4 x 96 well plates	400 mg	5.0 mL



---

## 5. Labeling of cells with EdU

- 5.1. Suspend the cells in an appropriate tissue culture medium to obtain optimal cell growth conditions. Please note that the growth of the cells during incubation decelerates, if the temperature changes or the cells are washed prior to incubation with EdU.
- 5.2. For the desired final concentration, add the appropriate amount of EdU to the culture medium and mix well. We recommend using a concentration of 10  $\mu$ M for 1 - 4 hours as a starting point. Use higher EdU concentrations for a shorter incubation time. A longer incubation time requires lower EdU concentrations.
- 5.3. The incubation of the cells with EdU should be performed under the optimal conditions for your cell type, the number of cells plated and for the desired length of time. Various DNA synthesis and proliferation parameters can be evaluated by altering the EdU incubation time or by subjecting the cells to pulse labeling with EdU. Effective time intervals for pulse labeling and the length of each pulse depend on the cell growth rate and the number of cells used.
- 5.4. If performing antibody surface labeling, proceed immediately to step 6, otherwise continue to step 7.

## 6. *Staining cell-surface antigens with antibodies (optional)*

- 6.1. Wash cells in each well with 100  $\mu$ L of 1% BSA in PBS.
- 6.2. Remove the wash solution and add again 100  $\mu$ L of 1% BSA in PBS to the cells.
- 6.3. Add surface antibodies and mix well but gently.  
  
**Note:** PE, PE-tandem or Quantum Dot antibody conjugates should not be used before performing the click reaction (step 8).
- 6.4. Incubate the cells for the recommended length of time and temperature. Protect from light!
- 6.5. Proceed to step 7.

## 7. Cell fixation and permeabilization

This protocol was developed with a fixation step using 4% Paraformaldehyde in PBS, followed by permeabilization step. A saponin-based permeabilization solution can be used with cell samples containing red blood cells or whole blood as well as with cell probes containing different cell types. The morphological light scatter characteristics of leukocytes are maintained by a saponin-based solution while red blood cells are lysed.

- 7.1.** Remove the incubation media and wash the cells, each well with **100 µL of 1% BSA in PBS**. Afterwards remove the wash solution.
- 7.2.** Add **100 µL of the fixative solution** to the cells in each well. Incubate for **15 minutes at room temperature**. Protect from light.
- 7.3.** Remove the fixation solution and wash the cells in each well twice with **200 µL of 1% BSA in PBS**. If red blood cells or haemoglobin are present in the sample, repeat the washing step. Remove all residual blood cell debris and haemoglobin before proceeding.

**NOTE:** At this point of the procedure, the probes can be stored safely.

- 7.4.** Remove the wash solution and add to each well **100 µL of permeabilization solution**. Mix well but gently, incubate for **20 minutes at room temperature** and proceed to step **8.** for the click reaction.

## 8. EdU detection

- 8.1.** Prepare the click assay cocktail in the same order as described in **Table 5**. If the ingredients are not added in the order listed, the reaction will not proceed optimally or might even fail.

**Important:** Once the assay cocktail is prepared, use it immediately, at least within the next 15 minutes!

Table 5: Click assay cocktails

Material	Component code	Number of 96 well plates		
		1	2	4
Reaction buffer	RP	9.447 mL	18.89 mL	37.78 mL
Reactor system	C - green	440 µL	880 µL	1760 µL
Dye Azide	D - red	23 µL	46 µL	92 µL
Buffer additive (prepared in 4.3)	B	1.1 mL	2.2 mL	4.4 mL
Total Volume	-	<b>11.01 mL</b>	<b>22.02 mL</b>	<b>44.04 mL</b>

- 8.2. Remove permeabilization solution from step 7.4 and add 100  $\mu$ L of the click assay cocktail to each well and mix well but gently to distribute the assay solution evenly.
- 8.3. Incubate the click assay mixture for 30 minutes at room temperature. Protect from light!
- 8.4. From the 10x rinse solution prepare a 1x rinse solution by applying following table (Table 6). Add the appropriate amount of PBS (1x) (see Table 6) to the **component R** and mix well (To prevent crystallization, keep **component R** at room temperature at all times. If **component R** has crystallized, please warm up to dissolve again. Please see also “cautions”). This additional wash step with this special rinse buffer reduces unspecific, cell number dependent background signal. After use, store any remaining solution at RT. When stored as directed, this stock solution is stable for up to 6 months.

Table 6: Amounts of aqueous solution needed to dissolve the rinse buffer to the final work solution

Sensitive EdU HTS Kit	Volume of 10x rinse buffer	Dilution volume of 1x PBS
2 x 96 well plates	5.8 mL	52.2 mL
4 x 96 well plates	11.5 mL	103.5 mL

Remove Click assay cocktail and wash the cells in each well twice with 150  $\mu$ L with the 1x rinse solution prepared above.

- 8.5. Remove rinse solution. 100  $\mu$ L of 1% BSA in PBS is then given to the cells in each well.
- 8.6. If performing antibody surface or intracellular labeling, proceed immediately to step 9, otherwise continue to step 10.

## 9. Staining intracellular or surface antigens (optional)

- 9.1. Add antibodies against intracellular antigens or against surface antigens that use RPE, PR-tandem or Quantum Dot antibody conjugates. Mix well.
- 9.2. Incubate the cells for the time and temperature required for antibody staining. Protect from light.
- 9.3. Wash each well twice with 100  $\mu$ L permeabilization solution. Remove the solution. Add again 100  $\mu$ L of 1% BSA in PBS to the cells.
- 9.4. Proceed with step **10** for analysing the cells.

## 10. Imaging and analysis

- 10.1. Close the 96 well plate by using a sealing film, if desired.
- 10.2. Fluorescence is quantified by scanning the plate using an automated imaging platform equipped with filters appropriate for the dye used. Images of each well can be taken by microscopy.

The excitation and emission maxima of the available dyes are listed in **Table 7**.

Table 7: Emission and excitation maxima of the available dyes.

Product number	Dye	Excitation (nm)	Emission (nm)	Filter
BCK-EdUPro488HTS2 ----- BCK-EdUPro488HTS4	Eterneon <sup>2</sup> GREEN Azide (Enhancer system – incl. FITC alternative)	496	516	green
BCK-EdUPro555HTS2 ----- BCK-EdUPro555HTS4	Eterneon <sup>2</sup> YELLOW Azide (Enhancer system – incl. Cy3 Azide alternative)	546	579	yellow