

OVENS and INCUBATORS



User Manual



Index

1	Warranty	1
2	Contents of package	1
3	First use	1
3.1	Getting started	1
3.2	Instrument parts	1
4	Display and commands	2
5	Instrument versions	3
6	Operation (Basic version)	4
6.1	Switching on the instrument	4
6.2	Setting of parameters	4
6.2.1	Working temperature	4
6.2.2	Working time	4
6.2.3	Fan speed (forced air instruments only)	4
6.3	Start/stop heating cycle	5
6.4	Functions with password access	5
6.4.1	Access to menu with password	5
6.4.2	Delay of heating cycle start	5
6.4.3	Safety temperature limiter for samples protection	6
6.4.4	Restart mode after absence of power supply	6
6.4.5	Temperature range for over temperature alarm	7
6.4.6	Temperature offset on single point, on entire ramp, on room temperature sensor	7
7	Operation (Professional version)	9
7.1	Switching on the instrument	9
7.2	Programming	9
7.2.1	Calling programs	9
7.2.2	Modify a program	9
7.3	Start/stop of a program	10
7.4	Functions with password access	10
7.4.1	Access to menu with password	10
7.4.2	Number of program to which apply the Delay and Cycle functions	11
7.4.3	Ripetition of a program	11
7.4.4	Delay of the program start	11
7.4.5	Safety temperature limiter for samples protection	12
7.4.6	Restart mode after absence of power supply	12
7.4.7	Temperature range for over temperature alarm	13
7.4.8	Temperature offset on single point, on entire ramp, on room temperature sensor	13
8	Clean and maintenance	14
9	Disposal of electronic equipment	14
9.1	Technical specifications and service	14

1 Warranty

Thank you for purchasing a product from Phoenix Instrument GmbH. In normal use conditions, the instrument is guaranteed for a period of 24 months from the date of purchase.

The warranty is valid only if the product is original. It does not apply to any product or parts of it that have been damaged due to incorrect installation, improper connections, improper use, accident or abnormal conditions of operation. The manufacturer declines all responsibility for damage caused by failure to follow instructions, lack of maintenance and any unauthorized modification

2 Contents of package

The instrument is delivered complete with the following parts:

1. n. 2 stainless steel wire shelves
2. n. 4 brackets for shelves
3. Power supply cable
4. User manual

3 First use


3.1 Getting started

The oven should be installed in follow conditions:

1. Dry, clean and stable work table with a flat horizontal surface
2. Respect minimum spaces around instrument 30-50 cm
3. Room temperature between 5 °C and 40 °C, and relative humidity maximum of 85%
4. Power supply socket with earth connection
5. Power feed between 220-240 V - 50 Hz

3.2 Instrument parts

Picture 1

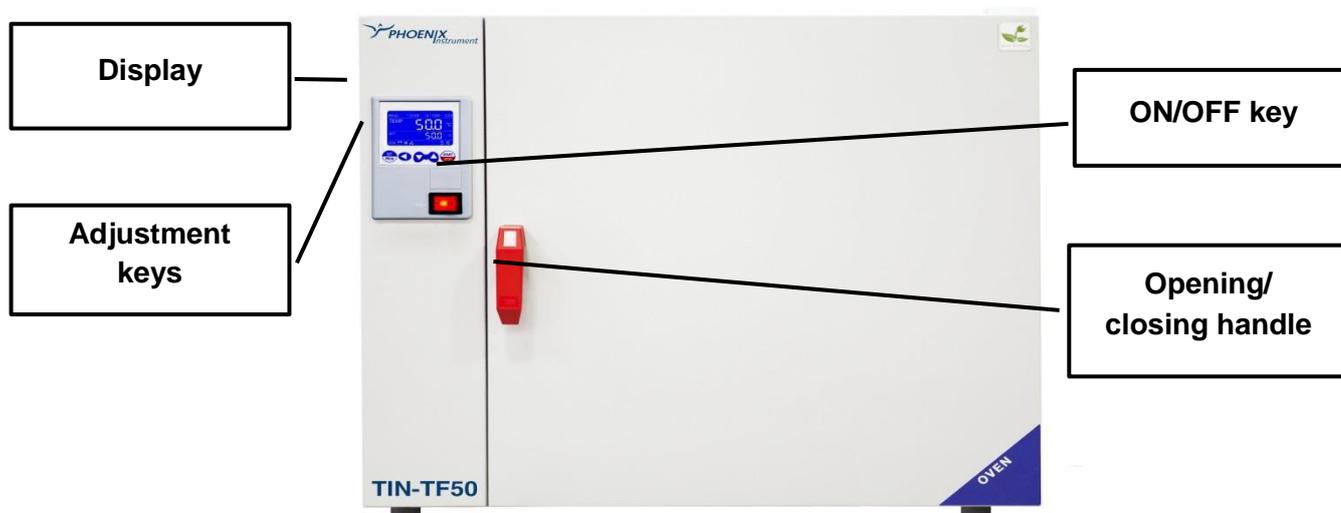


4 Display and commands



Picture 2 – BASIC version



Picture 3 - PROFESSIONAL (PRO) version

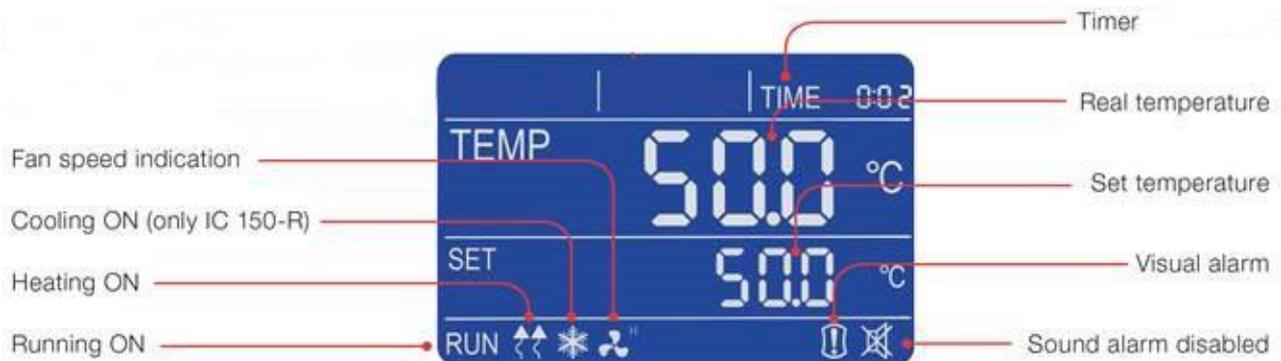

Picture 4 – Display BASIC version



Picture 5 - Display PROFESSIONAL (PRO) version

COMMANDS	DESCRIPTION
	The SET/PROG button permits the working parameters setting and to enter/escape from the programs (PRO version only). In combination with the SHIFT key allows access to menus with password (see paragraph 6.4).
	The SHIFT button permits to change quickly the digit (decimal, units, tens, etc.) of the value of the parameter you are editing. In combination with the SET/PROG key allows access to menus with password (see paragraph 6.4).
	Adjustment buttons allow you to increase or decrease the value of the operating parameter being edited.
	The START / STOP button permits to start / stop a cycle operation or a program (PRO version only).
	The ON/OFF button allows to turn on and turn off the instrument.

5 Instrument versions

The instruments are sold in two versions: BASIC (without programming) and PROFESSIONAL (with programming).

Depending the purchased version please follow this manual in the appropriate sections:

- **BASIC** (paragraph 6 at page 4)
- **PROFESSIONAL** (paragraph 7 at page 9)

6 Operation (Basic version)

6.1 Switching on the instrument

Connect the power cord to a power outlet with a protective ground connection.

Turn on the instrument by pressing the button ON / OFF. Button and the display will light up.

The display shows the initialization sequence and then the instrument is ready for use.

NOTE: every time you turn the instrument beeps intermittently, the icon of visual alarm  and the word "end" appear on the display, indicating that a heating cycle had been done before. Press any button to silence the audible signal and the icon  appears.

6.2 Setting of parameters

6.2.1 Working temperature

When the instrument is switched on, pressing one time the SET/PROG  button, the set temperature value starts to blink.

Set the desired temperature value (in Celsius degrees) pressing  keys.

It's possible a quick movement between the digits using the SHIFT  button.

Confirm the set value with another press of SET/PROG  button.

6.2.2 Working time

After confirming the temperature, the last value of the set time (timer) starts flashing.

Set the desired value (hh:mm) by pressing  keys. It's possible a quick movement between the digits using the SHIFT  button.

Confirm the set value with another press of SET/PROG  button.

NOTE: the value "00:00" indicates the operating mode "continuous", that means once you start the operating cycle by the START / STOP  button, it continues maintaining the set temperature until it is stopped manually (START/STOP ).

If you set a value of time, such as 1 hour, the instrument will reach the set temperature and will maintain it for an hour.

6.2.3 Fan speed (forced air instruments only)

After confirming the desired timer, the icon  starts to blink indicate the last level of fan speed selected H = High (100%), M = Medium (75%), L = Low (50%). Set the desired level by pressing the keys .

Confirm the set value with another press of SET/PROG  button.

6.3 Start/stop heating cycle

After setting the operating parameters, pressing START / STOP  button with long pressure (4-5 seconds), the heating cycle starts for the defined time in hh:mm or continuous (00:00). The word "end" at the top right corner of display disappears, the message RUN appears in the bottom left corner and display shows contemporary: timer, temperature measured inside the chamber, set temperature and fan speed if present (see Picture 4Picture 4).

At any time you can always manually stop the cycle by pressing the START / STOP  button with long pressure (4-5 seconds).

Once the set time or after manual stop, the instrument beeps intermittently, the icon of visual alarm  and the word "end" appear on the display. Pressing any button it's possible to silence the audible signal and the icon  appears.

NOTE: the acoustic signal will not end until it is stopped by the operator, but the heating cycle is terminated so for the samples inside the instrument will remain exposed to the internal temperature the chamber.

6.4 Functions with password access

6.4.1 Access to menu with password

Simultaneously pressing the SET / PROG  and SHIFT  for few seconds, you can access some functions and parameters that are password protected.

To access these submenus and avoid mistakenly entering in the operating parameters setting, it is recommended to firstly press the SHIFT  key, keep it pressed, and then press the SET / PROG  for few seconds.

After have made this keys combination, on the right top part of display instead of word TIME, "Lk" (lock) appears close to "0000" (password).

Below the passwords and access sequence to the various parameters/functions.

PASSWORD	FUNCTION/ PARAMETER	DESCRIPTION
0000	dy	Delay of heating cycle start
0003	tm	Safety temperature limiter for samples protection
	Po	Restart mode after absence of power supply
	AL	Temperature range for over temperature alarm
	Pb	Temperature offset on single point
	PK	Temperature offset on the entire ramp
	PA	Temperature offset of the room temperature probe

6.4.2 Delay of heating cycle start

It's possible to set a delay (hour and minutes) of heating cycle start.

Please follow the instructions reported at paragraph 6.4.1 and confirm the "0000" password pressing shortly one time SET/PROG .

On the top right part of display the parameter "dy" (delay) appears close to value 00:00.

Set the desired delay value (hh:mm) pressing  keys. It's possible a quick movement between the digits using the SHIFT  button. Confirm the set value with another press of SET/PROG  button.

The display comes back to the standby screen (see Picture 4).

Pressing the START/STOP  button with long pressure (4-5 seconds) the instrument starts the work cycle but it doesn't immediately heat: the word "end" and the set delay time alternately blink on the top right part of display, counting the wait time until the real starting of heating.

Once the delayed time is passed the instrument starts to heat and the regular timer appears on display.

6.4.3 Safety temperature limiter for samples protection

The instrument has the possibility to limit the maximum work temperature for the samples protection from an erroneous setting of the working temperature.

Please follow the instructions reported at paragraph 6.4.1 and using the  keys set the "0003" password. It's possible a quick movement between the digits using the SHIFT  button.

Confirm the set value with another press of SET/PROG  button.

On the top right part of display the parameter "tm" (temperature max) and the maximum expected value for the kind of instrument (different for oven and incubator) appear.

Set the maximum temperature value you want the instrument doesn't exceed during work cycle by the  keys. It's possible a quick movement between the digits using the SHIFT  button.

Confirm the set value with another press of SET/PROG  button.

Example

If the set temperature for the work cycle is 100 °C and the safety temperature is fixed at 70°C, the instrument tries to achieve the set temperature (100°C), even if it's major than the safety temperature set in this menu (tm).

When the 70 degrees are achieved the instrument goes in alarm emitting an audible intermittent alarm (silence it pressing any keys) and the heating element doesn't receive power supply until to the temperature will go below the safety temperature (tm).

NOTE: the instrument tries in any moment to achieve the set work temperature; as a consequence, until it is bigger than the safety temperature (tm), it goes in over temperature alarm as described in the previous paragraph.

6.4.4 Restart mode after absence of power supply

It's possible to set the restart mode of the instrument after a power supply absence:

<i>Po</i> VALUE	DESCRIPTION
0	On return of the power supply, the instrument does not automatically resume the heating cycle, but you must manually restart.
1	On return of the power supply, the instrument automatically resumes operation from the beginning of the heating cycle interrupted
2	On return of the power supply, the instrument automatically resumes operation at the very point of the heating cycle in which it was interrupted

Please follow the instructions reported at paragraph 6.4.1 and using the  keys set the “0003” password. It’s possible a quick movement between the digits using the SHIFT  button.

Confirm the set value with another press of SET/PROG  button.

On the top right part of display the parameter “tm” (temperature max), pass to the next parameter “Po” (Power) pressing shortly SET/PROG .

Confirm pressing shortly another time SET/PROG . Set the desired value (0, 1, 2) pressing the  keys. Confirm pressing shortly SET/PROG .

6.4.5 Temperature range for over temperature alarm

The instrument has the opportunity to set the range of temperature over which it goes in over temperature alarm.

NOTE: even if this value is adjustable by the operator, it’s already set by factory and perfectly calibrated in function of instrument type, natural/forced air oven or incubator.

We recommend to do not change this value unless absolutely necessary, because temperature fluctuations more or less than the set one, especially in models with natural convection, are normal and thus reducing dramatically the value of AL, it would risk do go frequently and unnecessarily alarmed the instrument.

Please follow the instructions reported at paragraph 6.4.1 and using the  keys set the “0003” password. It’s possible a quick movement between the digits using the SHIFT  button.

Confirm the set value with another press of SET/PROG  button

On the top right part of display the parameter “tm” (temperature max), pass to the next parameters pressing shortly SET/PROG  more times.

Find the parameter AL (alarm), set the minimum temperature value above which you want the instrument goes in alarm pressing the  keys. It’s possible a quick movement between the digits using the SHIFT  button. Confirm the set value with another press of SET/PROG  button.

6.4.6 Temperature offset on single point, on entire ramp, on room temperature sensor

The instrument has the opportunity to set the offset value on a single temperature point, on the entire temperature ramp and on the room temperature sensor.

NOTE: even if these values are adjustable by the operator, they are already set by factory and perfectly calibrated with certified and referable Accredia measurement instruments.

We recommend that you do not change these values unless absolutely necessary, for example if after a check with digital certified thermometer you find a discrepancies between the reading of the instrument and the external thermometer.

Please follow the instructions reported at paragraph 6.4.1 and using the  keys set the “0003” password. It’s possible a quick movement between the digits using the SHIFT  button.

Confirm the set value with another press of SET/PROG  button

On the top right part of display the parameter “**tm**” (temperature max), pass to the next parameters pressing shortly SET/PROG  more times.

<i>PARAMETER</i>	<i>DESCRIPTION</i>
Pb	Changing this parameter you can correct the reading of PT100 sensor inside the instrument on one point temperature. The correction will therefore be attributable to one specific point.
PK	Changing this parameter you can correct the reading PT100 sensor inside the instrument over the entire temperature ramp, that is going to change the inclination of the ramp reading of the sensor.
PA	Changing this parameter you can correct the reading of environmental PT100 sensor installed on the instrument (only refrigerated versions) on only one temperature point. The correction will therefore be attributable to one specific point.

7 Operation (Professional version)

7.1 Switching on the instrument

Connect the power cord to a power outlet with a protective ground connection.

Turn on the instrument by pressing the button ON / OFF. Button and the display will light up.

The display shows the initialization sequence and then the instrument is ready for use.

NOTE: every time you turn the instrument beeps intermittently, the icon of visual alarm  and the word “end” appear on the display, indicating that a heating cycle had been done before. Press any button to silence the audible signal and the icon  appears.

7.2 Programming

In the Professional version the instrument can manage until 7 programs with 10 steps each one in which temperature, timer and fan speed (if present) are settable.

Moreover them, it's possible to set a simple work cycle at single work step, with temperature, timer and fan speed (if present). This is called “PROG 0” and it is equivalent what the instrument does in the Basic version.

7.2.1 Calling programs

When the instrument is switched on, in standby or during a work cycle both, pressing shortly one time the SET/PROG  button, the word “PROG” and the program number (see Picture 5) start to blink together.

Calling the desired program by the  keys. Confirm pressing shortly one time the SET/PROG  button. The selected program is ready to start.

7.2.2 Modify a program

To modify a program it's necessary keep pressed for few seconds the SET/PROG  button: the word “PROG” and the program number start to blink together and after some moment only the program number blinks.

Now it's possible to choose the desired program to be modified by the  keys and to confirm it by a short press of SET/PROG  button.

Then the instrument enters in the modification mode and the temperature value of the first step blinks together the word “PROG” to indicate that you are in programming phase.

STEP 1

Set by the  and SHIFT  keys the temperature value of the first step. Press shortly SET/PROG  to confirm it and pass to the next value (timer), always of the first STEP. Set by the  and SHIFT  keys the desired timer value of the first step and confirm by a short press of SET/PROG .

If the instrument is a forced air model, the next parameter to be set is the fan speed, adjustable by the  keys in (H=High, M=Medium, L=Low), otherwise you pass to STEP 2.

STEP 2

Set by the  and SHIFT  keys the temperature value of the second step. Press shortly SET/PROG  to confirm it and pass to the next value (timer), always of the second STEP. Set by the  and SHIFT  keys the desired timer value of the second step and confirm by a short press of SET/PROG .

If the instrument is a forced air model, the next parameter to be set is the fan speed, adjustable by the  keys in (H=High, M=Medium, L=Low), otherwise you pass to STEP 3.

REPEAT THE ABOVE INSTRUCTIONS FOR EVERY STEP YOU WANT TO PROGRAM

NOTE: if you do not want to use all 10 STEP of the program you are editing, it is necessary to communicate to the instrument the end of the program. To do this, simply set in the next step after the last step you want to use the time equal to "00:00".

EXAMPLE

If the last work step you want to use is the fifth, it's sufficient set in the sixth step the timer equal to "00:00", imposing in this way to the instrument to stop it at the end of the fifth step.

NOTE: to modify the program 0, recall it as explained in paragraph 7.2.1 and proceed to the various parameters (temperature, timer and fan speed when present) as shown in paragraph 6.2 of the Basic version.

7.3 Start/stop of a program

After setting the program, simply call one of them and press the START / STOP  with long pressure (4-5 seconds) to start the selected program.

The word "end" at the top right of the display disappears, the message RUN appears on bottom left part and display shows simultaneously: program number, step in progress, timer, measured temperature inside the chamber, set temperature and fan speed if present (see Picture 5).

At any time you can always manually stop the cycle by pressing the START / STOP  button with long pressure (4-5 seconds).

Once the set program is finished or after a manual stop, the instrument beeps intermittently, the icon of visual alarm  and the word "end" appear on the display. Pressing any button will silence the audible signal and the icon  appears.

NOTE: the acoustic signal will not end until it is stopped by the operator, but the heating cycle is terminated so for the samples inside the instrument will remain exposed to the internal temperature the chamber.

7.4 Functions with password access

7.4.1 Access to menu with password

Simultaneously pressing the SET / PROG  and SHIFT  for few seconds, you can access some functions and parameters that are password protected.

To access these submenus and avoid mistakenly entering in the operating parameters setting, it is recommended to firstly press the SHIFT  key, keep it pressed, and then press the SET / PROG  for few seconds.

After have made this keys combination, on the right top part of display instead of word TIME, “Lk” (lock) appears close to “0000” (password). Below the passwords and access sequence to the various parameters/functions.

PASSWORD	FUNCTION/ PARAMETER	DESCRIPTION
0000	Pn	Number of program to which to apply the dy e Cy functions
	Cy	Number of repetitions of the work cycle
	dy	Partenza ritardata del programma selezionato
0003	tm	Safety temperature limiter for samples protection
	Po	Restart mode after absence of power supply
	AL	Temperature range for over temperature alarm
	Pb	Temperature offset on single point
	PK	Temperature offset on the entire ramp
	PA	Temperature offset of the room temperature probe

7.4.2 Number of program to which apply the Delay and Cycle functions

On the contrary of the Basic version that doesn't have more programs but a unique work cycle, in the Professional version it's necessary to define to which program (from 1 to 7) apply the functions of starting delayed (Delay) and repetition of cycle (Cycle).

To do that it's necessary enter in the first submenu with password access (0000) and modify the parameter Pn (program number) by  keys and confirm the selected program by a short press of SET/PROG  button.

7.4.3 Ripetition of a program

The instrument allows the repeating from one to more times of the selected program. After have chosen the program to which apply the function by the parameter Pn it's possible set the Cy value (Cy)= 1, 2, 3,...with  keys and SHIFT  and confirm it pressing shortly SET/PROG .

NOTE: it's also possible set the continuous repetition of a program, setting it in continuous “loop”, with the parameter Cy=0.

7.4.4 Delay of the program start

It's possible to set a delay (hour and minutes) of the program start.

After have chosen the program to which apply the function by the parameter Pn it's possible set the desired delay value (hh:mm) pressing  keys. It's possible a quick movement between the digits using the SHIFT  button. Confirm the set value with another press of SET/PROG  button. The display comes back to the standby screen (see Picture 5). Pressing the START/STOP  button with long pressure (4-5 seconds) the instrument starts the program but it doesn't immediately heat: the word “end” and the set delay time alternately blink on the top right part of display, counting the wait time until the real starting of the program.

Once the delayed time is passed the instrument starts to heat and the regular timer appears on display.

7.4.5 Safety temperature limiter for samples protection

The instrument has the possibility to limit the maximum work temperature for the samples protection from an erroneous setting of the working temperature.

Please follow the instructions reported at paragraph 6.4.1 and using the  keys set the "0003" password. It's possible a quick movement between the digits using the SHIFT  button.

Confirm the set value with another press of SET/PROG  button.

On the top right part of display the parameter "tm" (temperature max) and the maximum expected value for the kind of instrument (different for oven and incubator) appear.

Set the maximum temperature value you want the instrument doesn't exceed during work cycle by the  keys. It's possible a quick movement between the digits using the SHIFT  button.

Confirm the set value with another press of SET/PROG  button.

Example

If the set temperature for the work cycle is 100 °C and the safety temperature is fixed at 70°C, the instrument tries to achieve the set temperature (100°C), even if it's major than the safety temperature set in this menu (tm).

When the 70 degrees are achieved the instrument goes in alarm emitting an audible intermittent alarm (silence it pressing any keys) and the heating element doesn't receive power supply until to the temperature will go below the safety temperature (tm).

NOTE: the instrument tries in any moment to achieve the set work temperature; as a consequence, until it is bigger than the safety temperature (tm), it goes in over temperature alarm as described in the previous paragraph.

7.4.6 Restart mode after absence of power supply

It's possible to set the restart mode of the instrument after a power supply absence:

<i>Po</i> VALUE	DESCRIPTION
0	On return of the power supply, the instrument does not automatically resume the heating cycle, but you must manually restart.
1	On return of the power supply, the instrument automatically resumes operation from the beginning of the heating cycle interrupted
2	On return of the power supply, the instrument automatically resumes operation at the very point of the heating cycle in which it was interrupted

Please follow the instructions reported at paragraph 6.4.1 and using the  keys set the "0003" password. It's possible a quick movement between the digits using the SHIFT  button.

Confirm the set value with another press of SET/PROG  button.

On the top right part of display the parameter "tm" (temperature max), pass to the next parameter "Po" (Power) pressing shortly SET/PROG .

Confirm pressing shortly another time SET/PROG . Set the desired value (0, 1, 2) pressing the  keys. Confirm pressing shortly SET/PROG .

7.4.7 Temperature range for over temperature alarm

The instrument has the opportunity to set the range of temperature over which it goes in over temperature alarm.

NOTE: even if this value is adjustable by the operator, it's already set by factory and perfectly calibrated in function of instrument type, natural/forced air oven or incubator.

We recommend to do not change this value unless absolutely necessary, because temperature fluctuations more or less than the set one, especially in models with natural convection, are normal and thus reducing dramatically the value of AL, it would risk do go frequently and unnecessarily alarmed the instrument.

Please follow the instructions reported at paragraph 6.4.1 and using the  keys set the "0003" password. It's possible a quick movement between the digits using the SHIFT  button.

Confirm the set value with another press of SET/PROG  button

On the top right part of display the parameter "tm" (temperature max), pass to the next parameters pressing shortly SET/PROG  more times.

Find the parameter AL (alarm), set the minimum temperature value above which you want the instrument goes in alarm pressing the  keys. It's possible a quick movement between the digits using the SHIFT  button. Confirm the set value with another press of SET/PROG  button.

7.4.8 Temperature offset on single point, on entire ramp, on room temperature sensor

The instrument has the opportunity to set the offset value on a single temperature point, on the entire temperature ramp and on the room temperature sensor.

NOTE: even if these values are adjustable by the operator, they are already set by factory and perfectly calibrated with certified and referable Accredia measurement instruments.

We recommend that you do not change these values unless absolutely necessary, for example if after a check with digital certified thermometer you find a discrepancies between the reading of the instrument and the external thermometer.

Please follow the instructions reported at paragraph 6.4.1 and using the  keys set the "0003" password. It's possible a quick movement between the digits using the SHIFT  button.

Confirm the set value with another press of SET/PROG  button

On the top right part of display the parameter "tm" (temperature max), pass to the next parameters pressing shortly SET/PROG  more times.

PARAMETER	DESCRIPTION
Pb	Changing this parameter you can correct the reading of PT100 sensor inside the instrument on one point temperature. The correction will therefore be attributable to one specific point.
PK	Changing this parameter you can correct the reading PT100 sensor inside the instrument over the entire temperature ramp, that is going to change the

	inclination of the ramp reading of the sensor.
PA	Changing this parameter you can correct the reading of environmental PT100 sensor installed on the instrument (only refrigerated versions) on only one temperature point. The correction will therefore be attributable to one specific point.

8 Clean and maintenance

Proper maintenance and cleaning of the instrument guarantee its good conditions.

The inner chamber of the instrument is made of stainless steel, so it can be cleaned with any detergent provided it is not aggressive and / or corrosive.

You should clean the inside and outside surfaces with a standard all-purpose cleaner sprayed on a soft cloth.

Before proceeding with any cleaning or decontamination, the user must ensure that the method used does not damage the instrument.

IMPORTANT:

If the instrument must be returned for service, it is necessary to provide for proper cleaning and possible decontamination by pathogens of the same.

It is also recommended to put the instrument in its original packaging to send it in for repairs and if it is missed it is necessary to provide to pack it properly in order to the transport.

Any damage caused from the incorrect shipping will not be covered by warranty.

9 Disposal of electronic equipment



The electrical and electronic equipment marked with this symbol may not be disposed of in landfills.

In accordance with EU Directive 2002/96/EC, the European users of electrical and electronic equipment have the opportunity to give back to the distributor or manufacturer upon purchase of a new one.

The illegal disposal of electrical and electronic equipment is punished with an administrative fine.

Technical Specifications

Natural convection oven	TIN-TN30	TIN-TN50	TIN-TN115	TIN-TN200
Usable Volume	30 Liters	50 Liters	115 Liters	200 Liters
Max. Temperature/Resolution	+200/0,1°C	+300/0,1°C	+300/0,1°C	+300/0,1°C
Temperature homogeneity at 150°C	±3,5°C	±3,5°C	±3,5°C	±4°C
Temperature variation at 150°C	±0,5°C	±0,5°C	±0,5°C	±0,7°C
Heating time at 150°C (min)	20	24	30	50
Timer	99:59/ continuous operation	99:59/ continuous operation	99:59/ continuous operation	99:59/ continuous operation
Internal Dimension (WxHxD) in mm	320 x 320 x 285	400 x 420 x 330	520 x 495 x 450	650 x 640 x 495
No. of shelves (standard/max)	2/4	2/5	2/6	2/9
Min. distance between shelves	50mm	50mm	50mm	50mm
Max. load of shelves (kg)	10	15	20	20
Voltage/Power	230V/700W	230V/1000W	230V/1900W	230V/2100W
External Dimension (WxHxD) in mm	460 x 660 x 530	660 x 630 x 470	790 x 750 x 600	915 x 905 x 600
Weight (kg)	40	53	74	103
Safety class	3.1	3.1	3.1	3.1

Forced Air oven	TIN TF-50	TIN-TF120	TIN-TF200	TIN-TF400
Volume	50 Liters	120 Liters	200 Liters	400 Liters
Max. Temperature/Resolution	+300/0,1°C	+300/0,1°C	+300/0,1°C	+300/0,1°C
Temp. homogeneity at 150°C	±2%	±2%	±2%	±2%
Temperature variation at 150°C	±0,3°C	±0,3°C	±0,4°C	±0,5°C
Heating time at 150°C (min)	14	16	18	20
Timer	99:59/continuous operation	99:59/continuous operation	99:59/continuous operation	99:59/continuous operation
Int. Dimension (WxHxD) in mm	400 x 415 x 310	520 x 530 x 435	645 x 650 x 495	1000 x 800 x 500
No. of shelves (standard/max)	2/5	2/7	2/9	2/10
Min. distance between shelves	50mm	50mm	50mm	50mm
Max. load of shelves (kg)	15	20	20	20
Voltage/Power	230V/980W	230V/1900W	230V/2400W	230V/3200W
Ext.Dimension (WxHxD) in mm	665 x 635 x 570	785 x 750 x 690	920 x 870 x 755	1260 x 1060 x 750
Weight (kg)	54	74	103	160
Safety class	3.1	3.1	3.1	3.1

Incubators	TIN-IN16	TIN-IN35	TIN-IN55
Volume	16 Liters	35 Liters	55 Liters
Max. Temperature/Resolution	+70/0,1°C	+70/0,1°C	+70/0,1°C
Temp. homogeneity at 37°C	±0,4°C	±0,4°C	±0,5°C
Temperature variation at 37°C	±0,3°C	±0,3°C	±0,3°C
Heating time at 37°C (min)	18	22	25
Timer	99:59/continuous operation	99:59/continuous operation	99:59/continuous operation
Int. Dimension (WxHxD) in mm	270 x 230 x 255	360 x 300 x 320	400 x 360 x 385
No. of shelves (standard/max)	2/6	2/6	2/5
Min. distance between shelves	25mm	30mm	50mm
Max. load of shelves (kg)	5	7,5	10
Voltage/Power	230V/85W	230V/125W	230V/250W
Ext. Dimension (WxHxD) in mm	505 x 370 x 400	595 x 440 x 460	635 x 500 x 545
Weight (kg)	23	33	42
Safety class	2	2	2

Incubators	TIN-IN120	TIN-IN200
Volume	120 Liters	200 Liters
Max. Temperature/Resolution	+70/0,1°C	+70/0,1°C
Temp. homogeneity at 37°C	±0,5°C	±0,5°C
Temperature variation at 37°C	±0,3°C	±0,3°C
Heating time at 37°C (min)	30	35
Timer	99:59/continuous operation	99:59/continuous operation
Int. Dimension (WxHxD) in mm	520 x 460 x 500	610 x 600 x 575
No. of shelves (standard/max)	2/7	2/9
Min. distance between shelves	50mm	50mm
Max. load of shelves (kg)	10	10
Voltage/Power	230V/350W	230V/600W
Ext. Dimension (WxHxD) in mm	755 x 610 x 645	850 x 755 x 710
Weight (kg)	61	77
Safety class	2	2

Service

When help needed, please contact your local distributor or the service department of Phoenix Instrument GmbH for technical support in the following ways:

Phoenix Instrument GmbH
Heinkelstraße 10
30827 Garbsen
05131/9081830
info@phoenix-instrument.de

Phoenix Instrument GmbH – Heinkelstraße 10 – 30827 Garbsen
Telefon 05131 90818-30 – info@phoenix-instrument.de